


Lab Name _____ Phone # _____

Acct. # _____ Patient Name _____
First Last


Address/Email _____ Deliver by 5 p.m. on See Reverse for Working Times

Enclosed with case: Impressions Models Bite Photos Other: _____


Rx Coping(s)/Substructure(s) Sintered Only (You stain & glaze)
 Build-up for porcelain support Finished Completely
 Indicate implant system _____ Implant diameter _____ mm

FINAL SHADE

 Indicate Shade Here _____

OCCUSAL STAINING
 None Light* Medium Dark

PRESENT TOOTH OR STUMP SHADE

 Indicate Shade Here _____

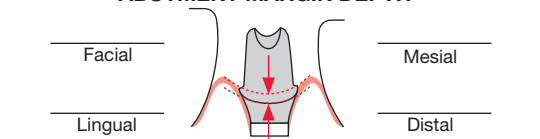
FINAL GINGIVAL SHADE
 G0 (Light) G1 (Standard)
 Ethnic: G3 (Med) G4 (Dark)


PONTIC DESIGN


SELECT RESTORATION TYPE
 BruxZir Full-Strength Solid Zirconia (1,150 MPa)
 BruxZir Full-Strength Screw-Retained (w/ Ti-Base)
 BruxZir Esthetic (870 MPa) (stump shade recommended for restorations less than 1.5 mm thick)
 BruxZir Esthetic Screw-Retained (w/ Ti-Base)
 BruxZir Full-Arch Implant Prosthesis pre-stained and sintered (you stain, glaze and cement inserts)
 BruxZir Full-Arch Implant Prosthesis completely finished
 Full-Arch PMMA Provisional Implant Prosthesis completely finished
 IPS e.max (anterior) IPS e.max (posterior)
 IPS e.max Screw-Retained (w/ Ti-Base)
 BioTemps Transition C&B Smile Transitions
 Abutment #(s) _____ Pontic #(s) _____
 Total Units _____
 Prismatic Clinical Zirconia Obsidian Fused to White Noble
 Obsidian Fused to Non-Precious Obsidian Fused to White High Noble

SELECT FINAL CUSTOM ABUTMENT
 Choose Material : Choose Brand
 Titanium* Inclusive*
 Gold-Colored Titanium BIOMET 3i Encode
 Zirconia w/ Ti-Base Straumann Variobase
 Gold Alloy
 Prepare existing abutment
See reverse for supported implant systems

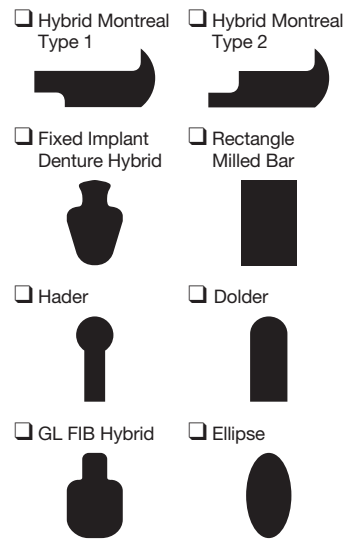
PARALLEL ABUTMENTS
 No Yes (indicate which abutments will have restorations splinted together for insertion)

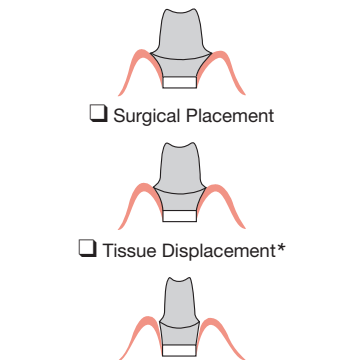
ABUTMENT MARGIN DEPTH

 If left blank, default values will be used

ABUTMENT MARGIN DESIGN

 Shoulder for all-ceramic* Chamfer for PFM/BruxZir*
***Standard unless specified otherwise**

SELECT BAR TYPE
INCLUSIVE IMPLANT BARS
 Locator CAD/CAM Milled Bar
 Screw-Retained Hybrid Bar

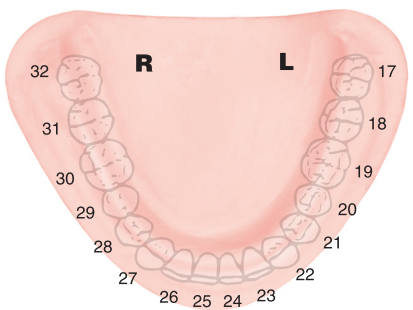
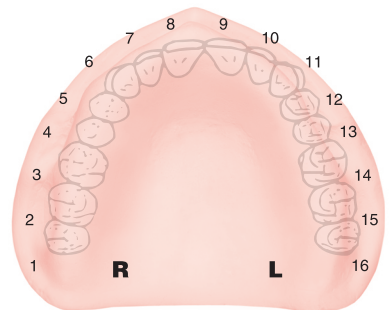
See reverse for supported implant systems



ABUTMENT EMERGENCE PROFILE

 Surgical Placement
 Tissue Displacement*
 No Tissue Displacement

Signature _____
 I verify that a signed prescription from a licensed dentist is on file for the restoration.
 See reverse for limited warranty details.

PLEASE COMPLETE THIS SECTION FOR IMPLANT BARS



(A-P Spread is 1.5 x A.P) First molar occlusion

DISTANCE BETWEEN ANTERIOR AND POSTERIOR IMPLANTS: _____ mm
 UPPER AP SPREAD X 1.5 mm: _____ mm

DISTANCE BETWEEN ANTERIOR AND POSTERIOR IMPLANTS: _____ mm
 LOWER AP SPREAD X 1.5 mm: _____ mm

IMPLANT WORKING TIMES

Please allow full working time for each product selected. Working times are NOT guaranteed and do NOT include weekends or holidays. Rush service available on most products but must be prescheduled (see below).

	<u>Days in Lab</u>
Inclusive Custom Abutments3
Encode Custom Abutments8
BruxZir restoration.....	.5
IPS e.max restoration5
Prismatik CZ restoration.....	.5
Obsidian restoration5
Full-cast restoration.....	.5
BruxZir Screw-Retained crown7
IPS e.max Screw-Retained crown.....	.7
Obsidian Screw-Retained crown.....	.7
BruxZir Full-Arch Implant Prosthesis pre-stained6
BruxZir Full-Arch Implant Prosthesis finished8
PMMA Full-Arch Implant Prosthesis finished.....	.6
Locator CAD/CAD-Milled Bar.....	.8
Screw-Retained Hybrid Bar.....	.8
BioTemps.....	.5
BioTemps cement over implant/cast-metal substructure/screw-retained6
Transition Crowns & Bridges5
Smile Transitions5

All rush cases must be prescheduled by calling **800-944-7874** before the case is shipped. Time of pickup and delivery may affect turnaround time.

TERMS AND WARRANTY INFORMATION



All Restorations
Made in the USA

We honor VISA, MASTERCARD, AMEX and DISCOVER.

TERMS: Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. **Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.** Prices subject to change without notice. Rx must be enclosed with original case submission.

NO-FAULT REMAKE POLICY: Glidewell Laboratories is pleased to process all remakes or adjustments at no additional charge if requested within the warranty period and accompanied by the return of the original appliance.

LIMITED WARRANTY/LIMITATION OF LIABILITY. For warranty terms and conditions and limitation of liability, visit glidewelldental.com/policies-and-warranties/.

INCLUSIVE® CUSTOM ABUTMENTS AND SCREW-RETAINED CROWNS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™ Certain®	CAMLOG® SCREW-LINE	Dentium® Implantium® SimpleLine® II SuperLine®	DENTSPLY Implants ANKYLOS® C/X ASTRA TECH Implant System®	Glidewell Direct Hahn™ Tapered Implant System Inclusive® Tapered Implant System	HIOSSSEN® HG System	
Keystone Dental PrimaConnex®	MegaGen AnyRidge® Implant System	Neoss® Neoss®	Nobel Biocare Brånemark System® RP NobelActive® NobelReplace®	Straumann® Bone Level Tissue Level	Sweden & Martina Premium Shelta	Zimmer Dental Screw-Vent®

INCLUSIVE® CAD/CAM MILLED IMPLANT BARS ARE COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™ Certain® External Hex (4.1mm)	DENTSPLY Implants ASTRA TECH Implant System®	Glidewell Direct Hahn™ Tapered Implant System Inclusive® Tapered Implant System	Keystone Dental PrimaConnex®	
MegaGen AnyRidge® Implant System	Neoss® Neoss® Implant System	Nobel Biocare Brånemark System® RP NobelActive® NobelReplace®	Straumann® Bone Level Tissue Level	Zimmer Dental Screw-Vent®

THE BRUXZIR® FULL-ARCH IMPLANT PROSTHESIS IS COMPATIBLE WITH THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™ Certain®	CAMLOG® SCREW-LINE	DENTSPLY Implants ANKYLOS® C/X ASTRA TECH Implant System®	Glidewell Direct Hahn™ Tapered Implant System Inclusive® Tapered Implant System		
HIOSSSEN® HG System	MegaGen AnyRidge® Implant System	Nobel Biocare Brånemark System® RP NobelActive® NobelReplace®	Straumann® Bone Level Tissue Level	Sweden & Martina Premium Shelta	Zimmer Dental Screw-Vent®

Inclusive is a registered trademark of Prismatik Dentalcraft, Inc. Hahn Tapered Implant is a trademark of Prismatik Dentalcraft, Inc. All other trademarks are property of their respective owners. Glidewell Laboratories works in partnership with Dentium, Keystone Dental, Neoss and Sweden & Martina. For Inclusive CAD/CAM milled implant bars, prices vary for Keystone Dental, MegaGen and Neoss. Dentium implant systems are limited to Inclusive Titanium Custom Abutments.